

525,005

10525005

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property
Organization
International Bureau



(43) International Publication Date
4 March 2004 (04.03.2004)

PCT

(10) International Publication Number
WO 2004/019275 A1

(51) International Patent Classification⁷: **G06T 5/00**

(21) International Application Number:
PCT/GB2003/003585

(22) International Filing Date: 18 August 2003 (18.08.2003)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
0219408.2 20 August 2002 (20.08.2002) GB

(71) Applicant (for all designated States except US): **MIRADA SOLUTIONS LIMITED** [GB/GB]; Oxford Centre for Innovation, Mill Street, Oxford OX2 0JX (GB).

(72) Inventors; and

(75) Inventors/Applicants (for US only): **MULET PARADA, Miguel** [ES/GB]; Mirada Solutions Limited, Oxford

Centre for Innovation, Mill Street, Oxford OX2 0JX (GB). **FELDMAR, Jacques** [FR/GB]; Mirada Solutions Limited, Oxford Centre for Innovation, Mill Street, Oxford OX2 0JX (GB). **DECLERCK, Jerome** [FR/GB]; Mirada Solutions Limited, Oxford Centre for Innovation, Mill Street, Oxford OX2 0JX (GB).


(74) Agents: **TYSON, Robin, Edward et al.**; J.A. Kemp & Co., 14 South Square, Gray's Inn, London WC1R 5JJ (GB).

(81) Designated States (*national*): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.

(84) Designated States (*regional*): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW),

[Continued on next page]

(54) Title: COMPUTATION OF CONTOUR

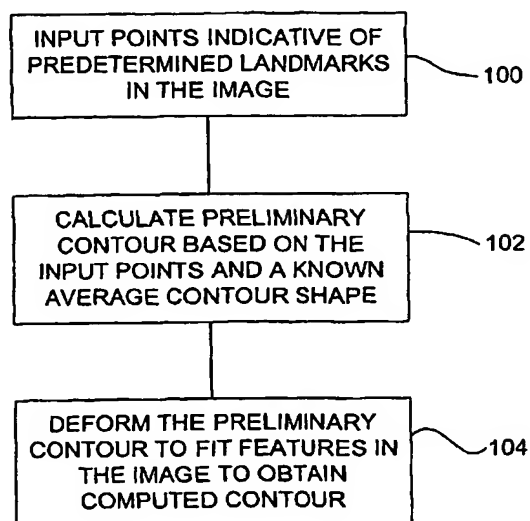

(57) **Abstract:** A method of computing a contour, such as the endocardial boundary in an ultrasound long-axis view of the heart, is disclosed. A plurality of points are input, each point being indicative of a predetermined landmark point in the image. A preliminary contour is then derived based on the input points and a known average contour shape which has been obtained from a database of contours derived from previous images. Finally, the preliminary contour is deformed to fit features identified in the image by a feature-extraction algorithm, to obtain the computed contour.

WO 2004/019275 A1



Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM),
European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE,
ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, RO,
SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM,
GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

Published:

— *with international search report*

COMPUTATION OF CONTOUR

The present invention relates to the computation of a contour, for example
5 representing the outline of an item of interest in an image.

A number of different techniques, also known as modalities, are now
available for creating medical images, for example tomographic images of the heart.
The left ventricle of the heart is the main pump which circulates oxygenated blood
around the body. Disorder and malfunction of the left ventricle is the main fatal
10 disease in western developed countries. Therefore assessment of the functioning of
the left ventricle has become of major importance.

Previously, one technique was to obtain images showing the heart moving
over a number of heart beats. These images are analysed by a cardiologist who
knows how to diagnose some diseases from a careful observation of the motion in the
15 images. Clearly this technique is time-consuming and depends on the skill and
experience of the cardiologist.

Other techniques attempt to analyse and quantify the performance of the heart
by identifying and tracking the motion of, for example, the endocardial boundary of
the left ventricle, i.e. the inner periphery of the wall of the left ventricle. Typically
20 the boundary is modelled as a smooth contour and the functional assessment would
be based on the analysis of the shape and the motion of the contour only.

One method of identifying the contour is to manually trace the boundary in
the image. This has the problems of being reliant on the skill of the user and is time-
consuming if it has to be performed on many images. If the contour is to be accurate
25 then a lot of points must be input.

Another technique which improves on this is to input fewer points on the
boundary, such as ten points which approximately trace the contour, then a computer
is used to fit a spline to the inputted points. Finally, known image processing
techniques are used to identify significant features in the image, including those
30 corresponding to the desired boundary, and an optimization technique is used to

adjust the spline to fit the boundary features in the image. Again, this technique suffers from the problems that, for it to work, a relatively large number of points must be input, and the final identified contour does not necessarily bear any relationship to the real-life anatomical properties of the item it represents, such as the
5 left ventricle.

Yet another technique is to create a database of known shapes of the item to be identified and to create a statistical model of the deformation of the shape. Image analysis is applied to the image to identify significant features and finally an optimization routine is used to find in the image the best contour which is a
10 compromise between the identified features and the statistical shape model. Further information on this method can be found in T.F. Cootes and C.J. Taylor "Statistical models of appearance for medical image analysis and computer vision", Proc. SPIE Medical Imaging 2001; Image Processing, Volume 4322, Editors Milan Sonka and Kenneth M. Hanson, July 2001, pp 236-248. This method suffers from the problem
15 that there is no information on how to initialise the search for the optimum contour in the image.

It is therefore an object of the invention to provide a technique for computation of a contour which alleviates, at least partially, any of the above problems.

20 Accordingly, the present invention provides a method of computing a contour comprising the steps of:

inputting a plurality of points, each point being indicative of a predetermined landmark point in an image;

25 deriving a preliminary contour based on the input points and a known average contour shape; and

deforming the preliminary contour to fit features identified in the image to obtain the computed contour.

The fact that the inputted points are indicative of predetermined landmark points means that the contour finding process is initialised and improves the
30 preliminary contour. The use of a preliminary contour based on a known average

contour shape means that it is necessary to input fewer points than previously because the derived contour will always be based on a known shape, and therefore, in the case of anatomical images enables the contour to be anatomically correct.

The use of *a priori* knowledge of the average shape of the contour of the item
5 of interest and the fact that the input points are known to correspond to specific landmarks, enables the number of input points to be far fewer than the number needed to define the shape of the computed contour, and the points do not have to be input specifically at regions of high curvature.

Preferably the number of inputted points is fewer than the number of points
10 needed to define the shape of the computed contour.

Preferably the number of degrees of freedom defined by the inputted points is fewer than the number of degrees of freedom needed to define the shape of the computed contour.

For computing a contour, there are basically 2 degrees of freedom per input
15 point. According to preferred embodiments of the invention, to define the shape of the final computed contour might require approximately 20 degrees of freedom, but the invention can achieve this using only, for example, 3 input points i.e. 6 degrees of freedom. In more detail, the number of degrees of freedom is related to the amount of information required from a user to obtain the contour of a desired shape. For
20 instance, it might take 10 points to achieve a visually acceptable contour using a standard parametric curve (e.g. linear interpolation between points, or a low-degree B-spline, such as quadratic or cubic, which is an extension of linear interpolation to a piecewise polynomial curve). These parametric curves are very commonly used, for example in graphics software for drawing free-form curves. A piecewise linear is a
25 very simplistic curve in the sense that in order to define the location anywhere along the curve you just need to know the 2 closest nodes (points) along the curve and draw a straight line between them. For a B-spline, it is not the 2 closest, but the 3 or 4 closest (for quadratic and cubic, respectively), so it is only slightly more sophisticated. However, the present invention is much more sophisticated because
30 there is a lot more information about the shape of the curve inside the definition of

the curve itself: this is what enables the user to input a minimal number of points. It is not necessary for the user to input all the information on the shape of the curve, e.g. by clicking a mouse at many points along the curve; instead much of the information is already stored in advance in the form of, for example, the average contour shape and a statistical shape model obtained from a database of known contours. Thus the invention enables the user to input only a few specific points to define the desired contour, and fewer points than would be required to define that contour from scratch. With a B-spline, you can draw whatever shape you want, but it takes a lot of points (degrees of freedom) to get it right. With embodiments of the invention you can draw only specific contours, for example left ventricular endocardiae (depending on the database used), but it requires only very few input points to do so.

The deriving step may comprise applying a parametric model to transform the known average contour shape such that the landmark points of the average contour shape match the corresponding input points. Preferably the deforming step comprises deforming the preliminary contour by applying the same parametric model as in the deriving step. The known average contour shape may be obtained using a database of contours derived from other images (typically previously collected images), and the parametric model can be a deformation model derived from a statistical shape model constructed from the same database of contours derived from previous images.

Preferably the image is an anatomical image, for example a long-axis view of the heart, and the computed contour can represent the endocardial boundary of the left ventricle of the heart. In this case it is only necessary to input three points which identify the following landmarks: the root of the left mitral valve leaflet, the apex of the left ventricle, and the root of the right mitral valve leaflet.

A further aspect of the present invention provides a method of computing the motion of a contour, for a temporal sequence of images of a subject, comprising the steps of:

computing the contour for one image of the sequence according to the method

described above;

using the computed contour as a new preliminary contour for a further image in the sequence;

deforming the new preliminary contour to fit features identified in the further
5 image to obtain the computed contour for the further image; and

repeating the using and deforming steps to obtain a computed contour for each image in the sequence.

The invention may be embodied in a computer system for processing data representing an image in conjunction with input points indicative of predetermined
10 landmark points and the invention extends to a computer program for executing the method on a programmed computer. The invention also extends to a computer program product carrying such a computer program.

Embodiments of the invention will be further described, by way of example only, with reference to the accompanying drawings in which:-

15 Figure 1 is a schematic illustration of the human heart in cross-section;

Figure 2 is a sketch of the left ventricle of the heart;

Figure 3 is a contrast enhanced ultrasound image of a long-axis view of the heart;

Figure 4 is the image of Figure 3 showing three identified landmark points
20 and a preliminary contour;

Figure 5 illustrates a set of points corresponding to significant locations in the image of Figure 3 extracted using a feature extraction algorithm;

Figure 6 is the ultrasound image of Figure 3 showing the final computed contour;

25 Figure 7 is a block diagram schematically showing a computer system for implementing the invention; and

Figure 8 is a flow diagram illustrating an embodiment of a method according to the invention.

In the different figures, corresponding parts are indicated by the same
30 reference numerals.

Embodiments of the present invention will be described with reference to the example of computing a contour of the endocardial boundary of the left ventricle of the human heart. Figure 1 is a sketch of the heart showing the four chambers, namely the right atrium 10, the right ventricle 12, the left atrium 14, and the left ventricle 16. Also indicated is the mitral valve of the left ventricle 16 comprising the right mitral valve leaflet 18 and the left mitral valve leaflet 20.

Figure 2 specifically shows the left ventricle 16, the shape of which is approximately a thick cup comprising the left ventricular muscle (myocardium) 22 surrounding the left ventricular cavity 24. At the closed end of the cup-shape is the apex 26 and at the opposite end there is located the right mitral valve leaflet 18 and the left mitral valve leaflet 20. The approximate axis of rotational symmetry of the left ventricle 16 is known as the long-axis 28.

Figure 3 is a tomographic image of the heart showing mainly the left ventricle 16. The image is a long-axis view i.e. a cross-sectional image in a plane substantially containing the long axis. The particular image in Fig. 3 is a contrast enhanced ultrasound image (echocardiogram). However, the invention can be used with images obtained by any other suitable modality, for example nuclear medicine, X-ray (fluoroscopy or ventriculography), magnetic resonance imaging and so on. The light region in the middle of the image of Figure 3 corresponds to the left ventricular cavity 24. The image in Figure 3 is the opposite way up to the diagram of Figure 2 in that in Figure 3 the apex 26 is at the top. The roots or bases of the left and right mitral valve leaflets are indicated at 30 and 32.

After data representing an image or sequence of images, such as Figure 3, have been obtained, the method of the invention can be applied. The apparatus for performing the method of the invention does not have to be part of the apparatus for obtaining the image and does not have to be operated by a sonographer or other radiographer. The apparatus for effecting the invention can be a conventional computer system which has access to the data representing the image or images to be analysed. Of course, the apparatus can be a system dedicated for use with the imaging equipment and can be operated by a radiographer. Figure 7 illustrates

schematically a computer system for computing a contour according to an embodiment of the invention. The software for performing a method embodying the invention is stored in data store 40 and executed by processor 42. Data corresponding to the image to be analysed can also be stored in data store 40 and
5 displayed by the processor 42 on display 44. An input device 46 enables the user to input information relating to the image on the display 44, as will be discussed in more detail below.

Figure 8 illustrates the contour computation method in accordance with an embodiment of the present invention. Firstly, in step 100 the user inputs three points
10 indicative of anatomical landmarks in the image. This can be conveniently done by viewing the image on the display 44 and using a mouse as the input device 46 to move a cursor on the display 44 and clicking a mouse button to input a point when the cursor is at a desired location. Any other suitable input device can be used in place of a mouse, for example a touch-sensitive screen, a stylus, a track-ball,
15 keyboard and so on. The data representing the points could have been entered previously by an operator, and stored, such that the "inputting" step 100 merely involves the processor 42 reading the data representing the points from a store.

In the present example, the three predetermined anatomical landmarks are the root of the left mitral valve, the apex, and the root of the right mitral valve leaflet.
20 Figure 4 shows the three input points as the light circles indicated at 50, 52 and 54, respectively. The three points can be input very quickly just by three mouse clicks. It is not necessary for the input points to be highly accurate, for example, an input point may just be indicative of the relevant landmark and could be anywhere within, for example, 5 mm of the landmark. The process by which the contour is obtained
25 and improved will be described below.

Next, according to step 102 of Figure 8, a preliminary contour is derived from the positions of the three input points. The preliminary contour 56 is shown in Figure 4. In order to generate such a contour 56 from just three points, and which contour is still anatomically plausible, a known average contour shape is used
30 together with a parametric model of the deformation which can transform the average

shape into any acceptable shape within a certain precision determined in advance. One way to do this is as follows. A database of contours is created, for example, by manually tracing the desired contour in many images, and for each contour of the database the three predetermined landmarks are identified, for instance by an expert.

- 5 The process of the creation of this database can be very labour-intensive, requiring much contribution by an expert, however, the database only needs to be created once and thereafter it can be used with a method according to this invention for the analysis of an unlimited number of new images. From the database of contours, an average contour can be computed. For example the contours are normalised with
- 10 respect to the variations of size and orientation of the left ventricle in the image, allowing the computation of the average shape.

Thereafter, continuing in step 102, the three landmark points of the real image and the three landmark points of the average shape contour are matched together, and a 2D similarity transformation (comprising rotation, translation and scaling) is

15 computed. The average contour is then deformed according to this similarity transformation to derive the preliminary contour 56 as shown in Figure 4. Further details of a way to create a statistical shape model from a database of real shapes for implementing the step just described are given in T.F. Cootes and C.J. Taylor "Statistical models of appearance for medical image analysis and computer vision",

20 proceedings SPIE Medical Imaging 2001; Image Processing, Volume 4322, Editors Milan Sonka and Kenneth M. Hanson, July 2001, pp 236-248. However, any other parametric model would be acceptable.

The preliminary contour 56 shown in Figure 4 has the generic shape of the left ventricle as it appears in a typical image of the same modality, and is close to the

25 real shape, but is not quite right.

Therefore in step 104 of the Figure 8, the preliminary contour 56 is deformed to match or better fit features in the real image. Figure 5 shows a set of points at significant locations in the image of Figure 3 obtained using a feature extraction algorithm. These features were extracted using the method explained in WO

30 02/43004, but any feature extraction algorithm which provides a discrete set of points

at significant locations in the image is suitable.

The preliminary contour obtained at step 102 is deformed using the adaptation of the iterative closest point (ICP) algorithm, for example as explained in M. Mulet Parada "Intensity independent feature extraction and tracking in echocardiographic sequences", PhD manuscript, Oxford University, Oxford, United Kingdom, 2000. Further information on the ICP algorithm can be gleaned from J. Declerck, J. Feldmar, M. L. Goris and F. Betting "Automatic registration and alignment on a template of cardiac stress and rest SPECT images", IEEE Transactions on Medical Imaging 16(6):727-737, December 1997. The transformation model which is used to deform the preliminary contour 56 can be, for example simple radial basis functions, or B-splines tensor product as in the reference by Declerck, Feldmar, Goris and Betting cited above, or preferably the same deformation model derived from a statistical shape model constructed from the contour database as explained above with reference to step 102 and in the publication by Cootes and Taylor. Figure 6 shows the computed contour 58 obtained as the result of step 104. The deformation of the preliminary contour 56 to obtain the computed contour 58 in step 104 is not constrained to the original three input points and hence the accuracy of the computed contour 58 is not dependent on the accuracy of the three input points, provided that the three input points are approximately in the vicinity of the predetermined landmark points in the image.

The computed contour 58 can be used as the basis for an automatic calculation of a single-plane estimate of the left ventricle volume using conventional integration techniques, such as a modified Simpson's rule or the method of discs. From an end diastolic image (i.e. at the end of cardiac relaxation), the end diastolic volume EDV can be obtained, and from an end systolic image (i.e. at the end of cardiac contraction), the end systolic volume ESV can be calculated. The difference between these volumes i.e. EDV minus ESV gives the stroke volume which is the estimated amount of blood ejected by the left ventricle, and the stroke volume divided by the end diastolic volume EDV gives the ejection fraction. The stroke volume and ejection fraction are important parameters in the assessment of the

function of the heart of a patient.

Typically a sequence of images is obtained at intervals of approximately one tenth of a second showing the heart, and in particular the left ventricle, moving over one or more heart beats. In analysing such a sequence according to a further
5 embodiment of the invention, it is not necessary for the user to input the landmark points for every image in the sequence. In fact, the three landmark points can be input for just one image in the sequence which is then used to obtain a computed contour according to a method of Figure 8 as described above. The computed contour can then be tracked through the image in each frame of the sequence, for
10 example as described in WO 02/43004, or for example, the computed contour could be used as a preliminary contour for repeating step 104 for each of the other images or using a contour computed for the image of one frame as the preliminary contour for the image of an adjacent frame and iterating through the sequence.

After the contour has been computed for each frame, an estimate of the
15 ventricle volume can be calculated for each frame and the maximum volume set as the end diastolic volume and the minimum volume in a sequence set as end systolic volume, and from these the ejection fraction and stroke volume can be calculated. This process can be entirely automated, such that for a sequence of images, just by performing a mouse click approximately at each of three landmark points in one
20 image, the ejection fraction and stroke volume can be obtained without any further user input.

Although the embodiments described above have been in terms of the human heart, this is purely by way of example, and the method of the invention can be applied to other organs, such as the brain or liver, in which case a different set of
25 predetermined landmarks would be used, and the number of landmark points would not necessarily be three. Any desired modality could also be used. The technique can be used with views of the heart other than the long-axis view, and again different landmarks would be determined in advance. The embodiments described above have given the example of computing a contour in 2 dimensions, but the invention is not
30 limited to 2D and can be used in further dimensions such as 3D.

-11-

The invention is also not limited to obtaining contours in anatomical or medical images and could equally be used in other fields, such as assisted object recognition, such as of vehicles or aircraft, fingerprinting, assisted segmentation of buildings in satellite image processing and so on.

CLAIMS

1. A method of computing a contour comprising the steps of:
inputting a plurality of points, each point being indicative of a predetermined
5 landmark point in an image;
deriving a preliminary contour based on the input points and a known average
contour shape; and
deforming the preliminary contour to fit features identified in the image to
obtain the computed contour.
10
2. A method according to claim 1, wherein the number of inputted points is fewer
than the number of points needed to define the shape of the computed contour.
3. A method according to claim 1 or 2, wherein the number of degrees of freedom
15 defined by the inputted points is fewer than the number of degrees of freedom needed
to define the shape of the computed contour.
4. A method according to claim 1, 2 or 3, wherein the known average contour shape
is obtained using a database of contours derived from previous images.
20
5. A method according to claim 1, 2, 3 or 4, wherein the deriving step comprises
applying a parametric model to transform the known average contour shape such that
the landmark points of the average contour shape match the corresponding input
points.
25
6. A method according to claim 5, wherein the deforming step comprises deforming
the preliminary contour by applying the same parametric model as in the deriving
step.
- 30 7. A method according to claim 5 or 6, wherein the parametric model is a

-13-

deformation model derived from a statistical shape model constructed from a database of contours derived from previous images.

8. A method according to any one of the preceding claims, wherein the contour
5 represents the boundary of an item of interest in the image.
9. A method according to any one of the preceding claims, wherein the image is an anatomical image.
- 10 10. A method according to claim 9, wherein the image is an image of the heart.
11. A method according to claim 10, wherein the image is a long-axis view of the heart.
- 15 12. A method according to claim 10 or 11, wherein the contour represents the endocardial boundary of the left ventricle of the heart.
13. A method according to claim 12, further comprising the step of calculating the volume of the left ventricle.
- 20 14. A method according to any one of claims 10 to 13, wherein the predetermined landmark points in the image comprise: the root of the left mitral valve leaflet, the apex of the left ventricle, and the root of the right mitral valve leaflet.
- 25 15. A method according to any one of the preceding claims, wherein the number of inputted points is exactly three.
16. A method according to any one of the preceding claims, wherein the image is an image created using a modality selected from the group consisting of ultrasound,
30 nuclear medicine, X-ray and magnetic resonance imaging.

17. A method of computing the motion of a contour, for a temporal sequence of images of a subject, comprising the steps of:

computing the contour for one image of the sequence according to the method of anyone of the preceding claims;

5 using the computed contour as a new preliminary contour for a further image in the sequence;

deforming the new preliminary contour to fit features identified in the further image to obtain the computed contour for the further image; and

10 repeating the using and deforming steps to obtain a computed contour for each image in the sequence.

18. A method according to claim 17, wherein the computed contours represent the endocardial boundary of the left ventricle of the heart, further comprising the steps of: calculating left ventricle volumes from the computed contours; using the

15 calculated volumes to calculate at least one of the stroke volume and ejection fraction of the heart.

19. A computer system comprising a data processor, a data storage means, input device and a display, the data processor being adapted to process data in accordance
20 with an executable program stored in the data storage means, wherein the executable program is adapted to execute the method of any one of the preceding claims on data representing the image displayed on the display and using the plurality of points indicative of predetermined landmark points in the image input with the input device.

25 20. A computer program comprising program code means for executing on a computer the method of any one of claims 1 to 18.

21. A computer program product carrying the computer program of claim 20.

Fig. 1

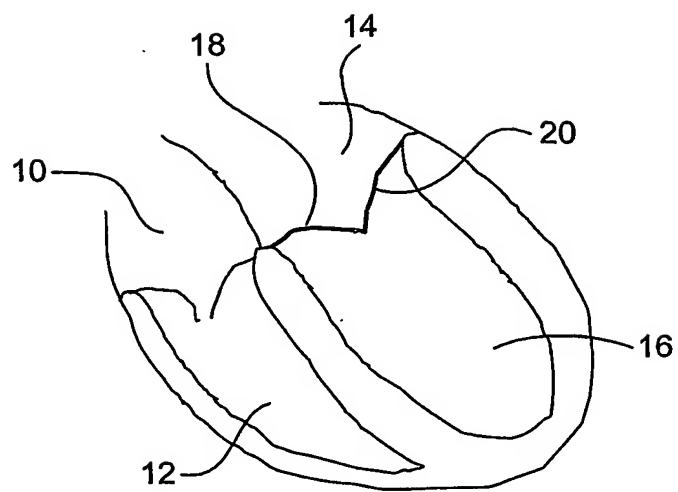


Fig. 2

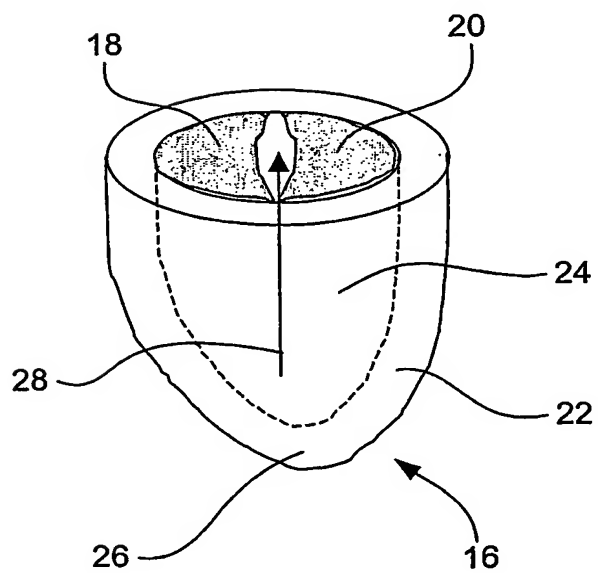


Fig. 3


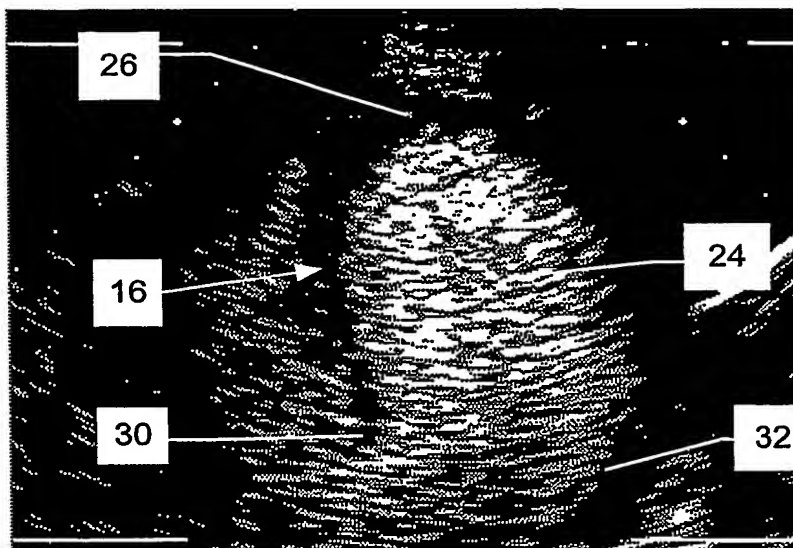


Fig. 4

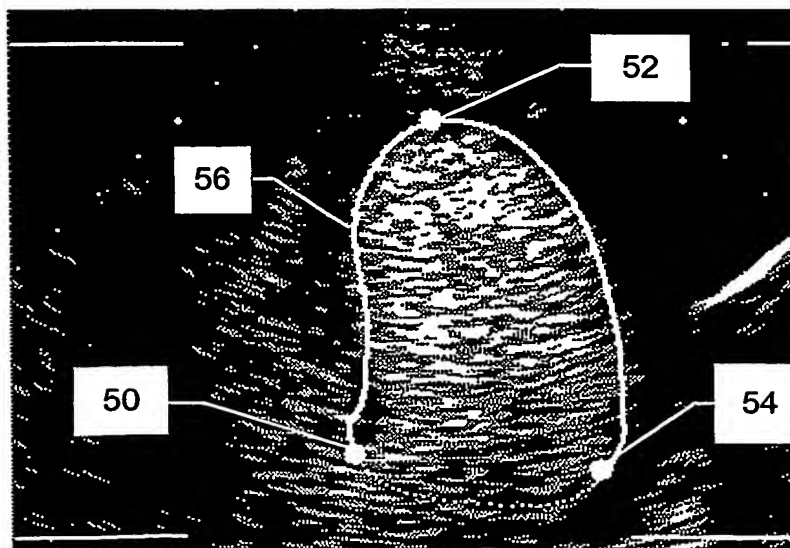

BEST AVAILABLE COPY

Fig. 5


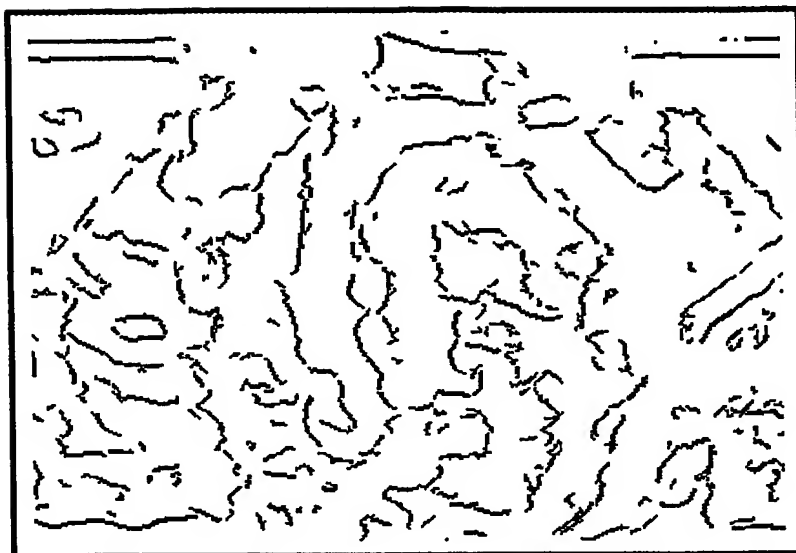


Fig. 6

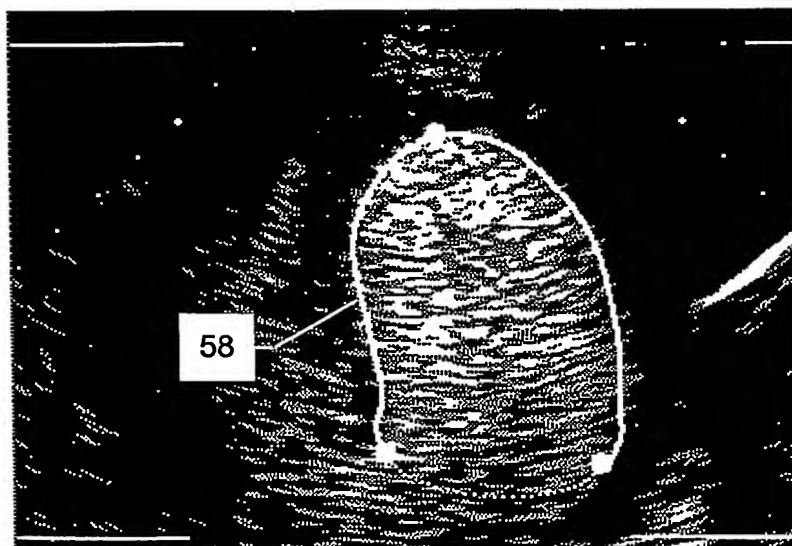

BEST AVAILABLE COPY

Fig. 7


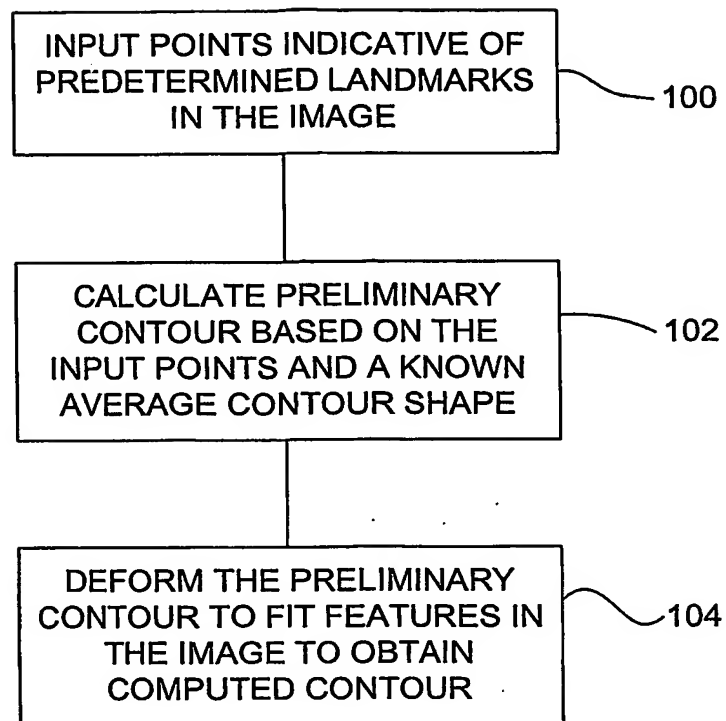


Fig. 8

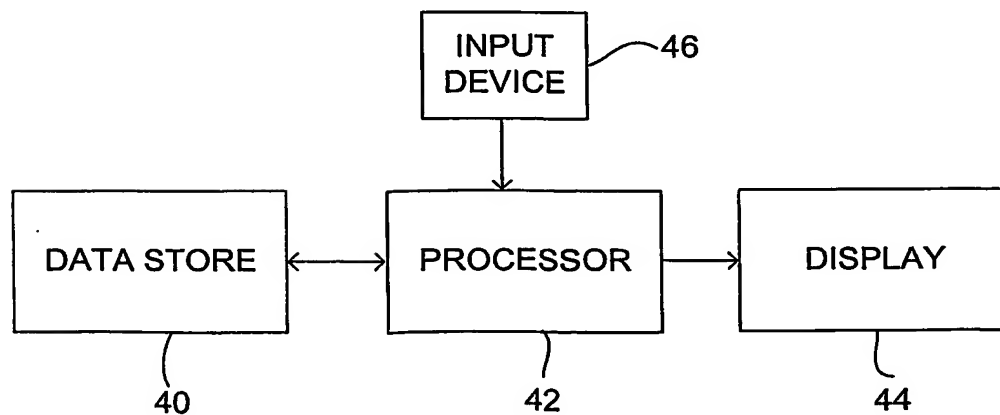

INTERNATIONAL SEARCH REPORT

Internal Application No

PCT/GB 03/03585

A. CLASSIFICATION OF SUBJECT MATTER
IPC 7 G06T5/00

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 G06T

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the International search (name of data base and, where practical, search terms used)

INSPEC, EPO-Internal, WPI Data

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	EP 1 076 318 A (JOHN P ROBARTS RES INST) 14 February 2001 (2001-02-14)	1-3,5,6, 8,9,16, 19-21
X	page 8, line 16 - line 32	17
Y	page 8, line 16 - line 32	18
Y	claim 1; figure 6	4,7, 10-15

	-/--	

☒ Further documents are listed in the continuation of box C.☒ Patent family members are listed in annex.

* Special categories of cited documents :

- *A* document defining the general state of the art which is not considered to be of particular relevance
- *E* earlier document but published on or after the international filing date
- *L* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- *O* document referring to an oral disclosure, use, exhibition or other means
- *P* document published prior to the international filing date but later than the priority date claimed

- *T* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- *X* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- *Y* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- * & * document member of the same patent family

Date of the actual completion of the international search

30 October 2003

Date of mailing of the international search report

06/11/2003

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Werling, A

INTERNATIONAL SEARCH REPORT

Internal Application No

PCT/GB 03/03585

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	COOTES T F ET AL: "Statistical models of appearance for medical image analysis and computer vision" MEDICAL IMAGING 2001: IMAGE PROCESSING, SAN DIEGO, CA, USA, 19-22 FEB. 2001, vol. 4322, pt.1-3, pages 236-248, XP009020085 Proceedings of the SPIE - The International Society for Optical Engineering, 2001, SPIE-Int. Soc. Opt. Eng, USA ISSN: 0277-786X cited in the application abstract	4,7
Y	MCINERNEY T ET AL: "Deformable Models in Medical Analysis: A Survey" MEDICAL IMAGE ANALYSIS, OXFORD UNIVERSITY PRESS, OXFORD, GB, vol. 1, no. 2, June 1996 (1996-06), pages 91-108, XP002230283 ISSN: 1361-8423 sec. 3.5, "Motion tracking and analysis" page 100 -page 101	10-15
Y	US 2002/102023 A1 (YAMAUCHI MASAKI) 1 August 2002 (2002-08-01) page 12, paragraph 202 -page 13, paragraph 204; figures 26,27	18
A	JAIN ET AL: "DEFORMABLE TEMPLATE MODELS: A REVIEW" SIGNAL PROCESSING. EUROPEAN JOURNAL DEVOTED TO THE METHODS AND APPLICATIONS OF SIGNAL PROCESSING, ELSEVIER SCIENCE PUBLISHERS B.V. AMSTERDAM, NL, vol. 71, no. 2, December 1998 (1998-12), pages 109-129, XP000858630 ISSN: 0165-1684 the whole document	1-21
A	COOTES T F ET AL: "Use of active shape models for locating structures in medical images" IMAGE AND VISION COMPUTING, JULY-AUG. 1994, UK, vol. 12, no. 6, pages 355-365, XP009020099 ISSN: 0262-8856 cited in the application the whole document	1-21

-/--

INTERNATIONAL SEARCH REPORT

Internat plication No
PCT/GB 03/03585

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT		
Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	DECLERCK J ET AL: "AUTOMATIC REGISTRATION AND ALIGNMENT ON A TEMPLATE OF CARDIAC STRESS AND REST REORIENTED SPECT IMAGES" IEEE TRANSACTIONS ON MEDICAL IMAGING, IEEE INC. NEW YORK, US, vol. 16, no. 6, 1 December 1997 (1997-12-01), pages 727-737, XP000738193 ISSN: 0278-0062 cited in the application the whole document	1-21
A	DE 198 57 608 A (DEUTSCHES KREBSFORSCH) 6 July 2000 (2000-07-06) figure 1	1-21
A	HILL A ET AL: "MEDICAL IMAGE INTERPRETATION: A GENERIC APPROACH USING DEFORMABLE TEMPLATES" MEDICAL INFORMATICA, TAYLOR AND FRANCIS, BASINGSTOKE, GB, vol. 19, no. 1, January 1994 (1994-01), pages 47-59, XP009004299 ISSN: 0307-7640 the whole document	1-21

INTERNATIONAL SEARCH REPORT

Internal Application No
PCT/GB 03/03585

Patent document cited in search report		Publication date		Patent family member(s)		Publication date
EP 1076318	A	14-02-2001	CA	2301675 A1		13-02-2001
			EP	1076318 A1		14-02-2001
US 2002102023	A1	01-08-2002	JP	2002224116 A		13-08-2002
DE 19857608	A	06-07-2000	DE	19857608 A1		06-07-2000
			AU	2277100 A		03-07-2000
			WO	0036563 A1		22-06-2000
			DE	19982719 D2		03-01-2002